
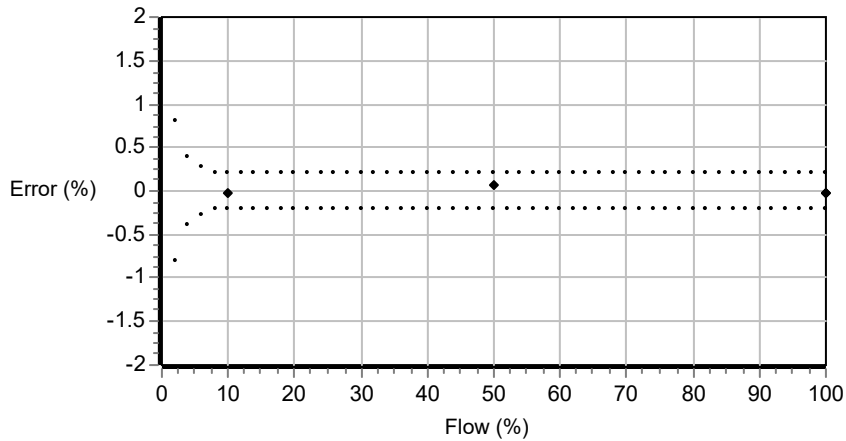


Product Code	Serial ID	Order ID	Line	Item	Customer Tag
F200SXXXC	14293415				



Process **Detail**

Process ID : 7.19421600 
Process Time : 2012.05.23 13:21:55
Process Stand : TSM2C@SSCC:1
Stand Uncertainty : +/-0.030%
Fluid : H2O
100% Rate : 725.7477 KG/MIN
Pickoff : 1
Max Rate P/T : 66.01 PSIG/22.5 C



Results

Status : PASS
D1 : 0
D2 : 1
K1 : 3376.488
K2 : 3886.343
DT : 4.5
FD : 6000
DTG : 0
DFQ1 : 0
DFQ2 : 0
FlowCal : 1533.94.56
FFQ : 0
FTG : 0
DensCal : 03376038864.50
FCF : 1533.9
FT : 4.56

Flow (%)	Flow Rate (kg/min)	Meter Total (kg)	Reference Total (kg)	Error (%)	Specification (±%)
100.0	725.7477	545.2542	545.4053	-0.028	0.200
10.0	72.57477	54.83992	54.8572	-0.031	0.200
50.0	362.8739	272.7844	272.5535	0.085	0.200
100.0	725.7477	547.0081	547.1091	-0.018	0.200

A. RUIZ
 Technician
 This certificate is produced by an electronic data system and is valid without signature.